



NOTES


1. Text: Black. Background: White.
2. Make from: Ventana P/N 07184603001, approximately 1.75 x 4.0".
3. The individual label file can be located in the Document Control System (DCS) under 07447485001b.btw.
4. Outside border line is shown here for illustrative purposes only and does not print.
5. Label image is shown here at an approximate size. Label dimensions are contained in the drawing of the label stock found on the bill of materials.
6. Lot Number, Expiry Date, barcodes, and barcode-related human readable text are shown here for illustrative purposes only. Actual data will vary by job.

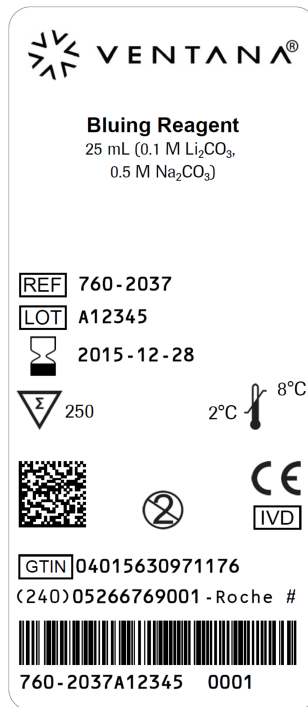

B	Update to latest revision of new template (OCRB font for LVS)	See Agile	KL	C048728
REV	DESCRIPTION	EFFECTIVE DATE	RP	CO
TITLE: LBL, 1 DSPNR BOX, 2DBC, FG 760-2037				
		This document contains confidential, proprietary information of Ventana Medical Systems, Inc. It may not be copied or reproduced without prior written permission from Ventana Medical Systems, Inc.		REV: B
Ventana Medical Systems, Inc. Tucson, Arizona		PART NUMBER: 07447485001	DMS MATERIAL NUMBER: 07447485001	SHEET 1 OF 1


NOTES:

1. Text: Black. Background: White.
2. Make from: Ventana P/N 1442800 blank label stock (DMS Mat. No. 05249368001), approximately 3.00 x 1.75".
3. The individual label file can be located in the Document Control System (DCS) under 07447817001b.btw.
4. Outside border line is shown here for illustrative purposes only and does not print.
5. Label image is shown here at an approximate size. Label dimensions are contained in the drawing of the label stock found on the bill of materials.
6. Lot Number, Expiry Date, and 2D barcode are shown here for illustrative purposes only. Actual data will vary by job.

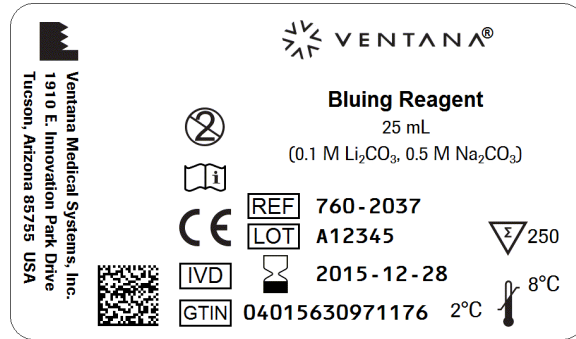


B	Update to latest revision of new template (OCR font for LVS)	See Agile	CB	C048729
REV	DESCRIPTION	EFFECTIVE DATE	RP	CO


TITLE: **LBL, 1 DSPNR BRL, 2DBC, 760-2037**

	This document contains confidential, proprietary information of Ventana Medical Systems, Inc. It may not be copied or reproduced without prior written permission from Ventana Medical Systems, Inc.		REV: B
Ventana Medical Systems, Inc. Tucson, Arizona	PART NUMBER: 07447817001	DMS MATERIAL NUMBER: 07447817001	SHEET 1 OF 1

NOTES:

- 1. COLOR SWATCHES
 - a.PMS 300

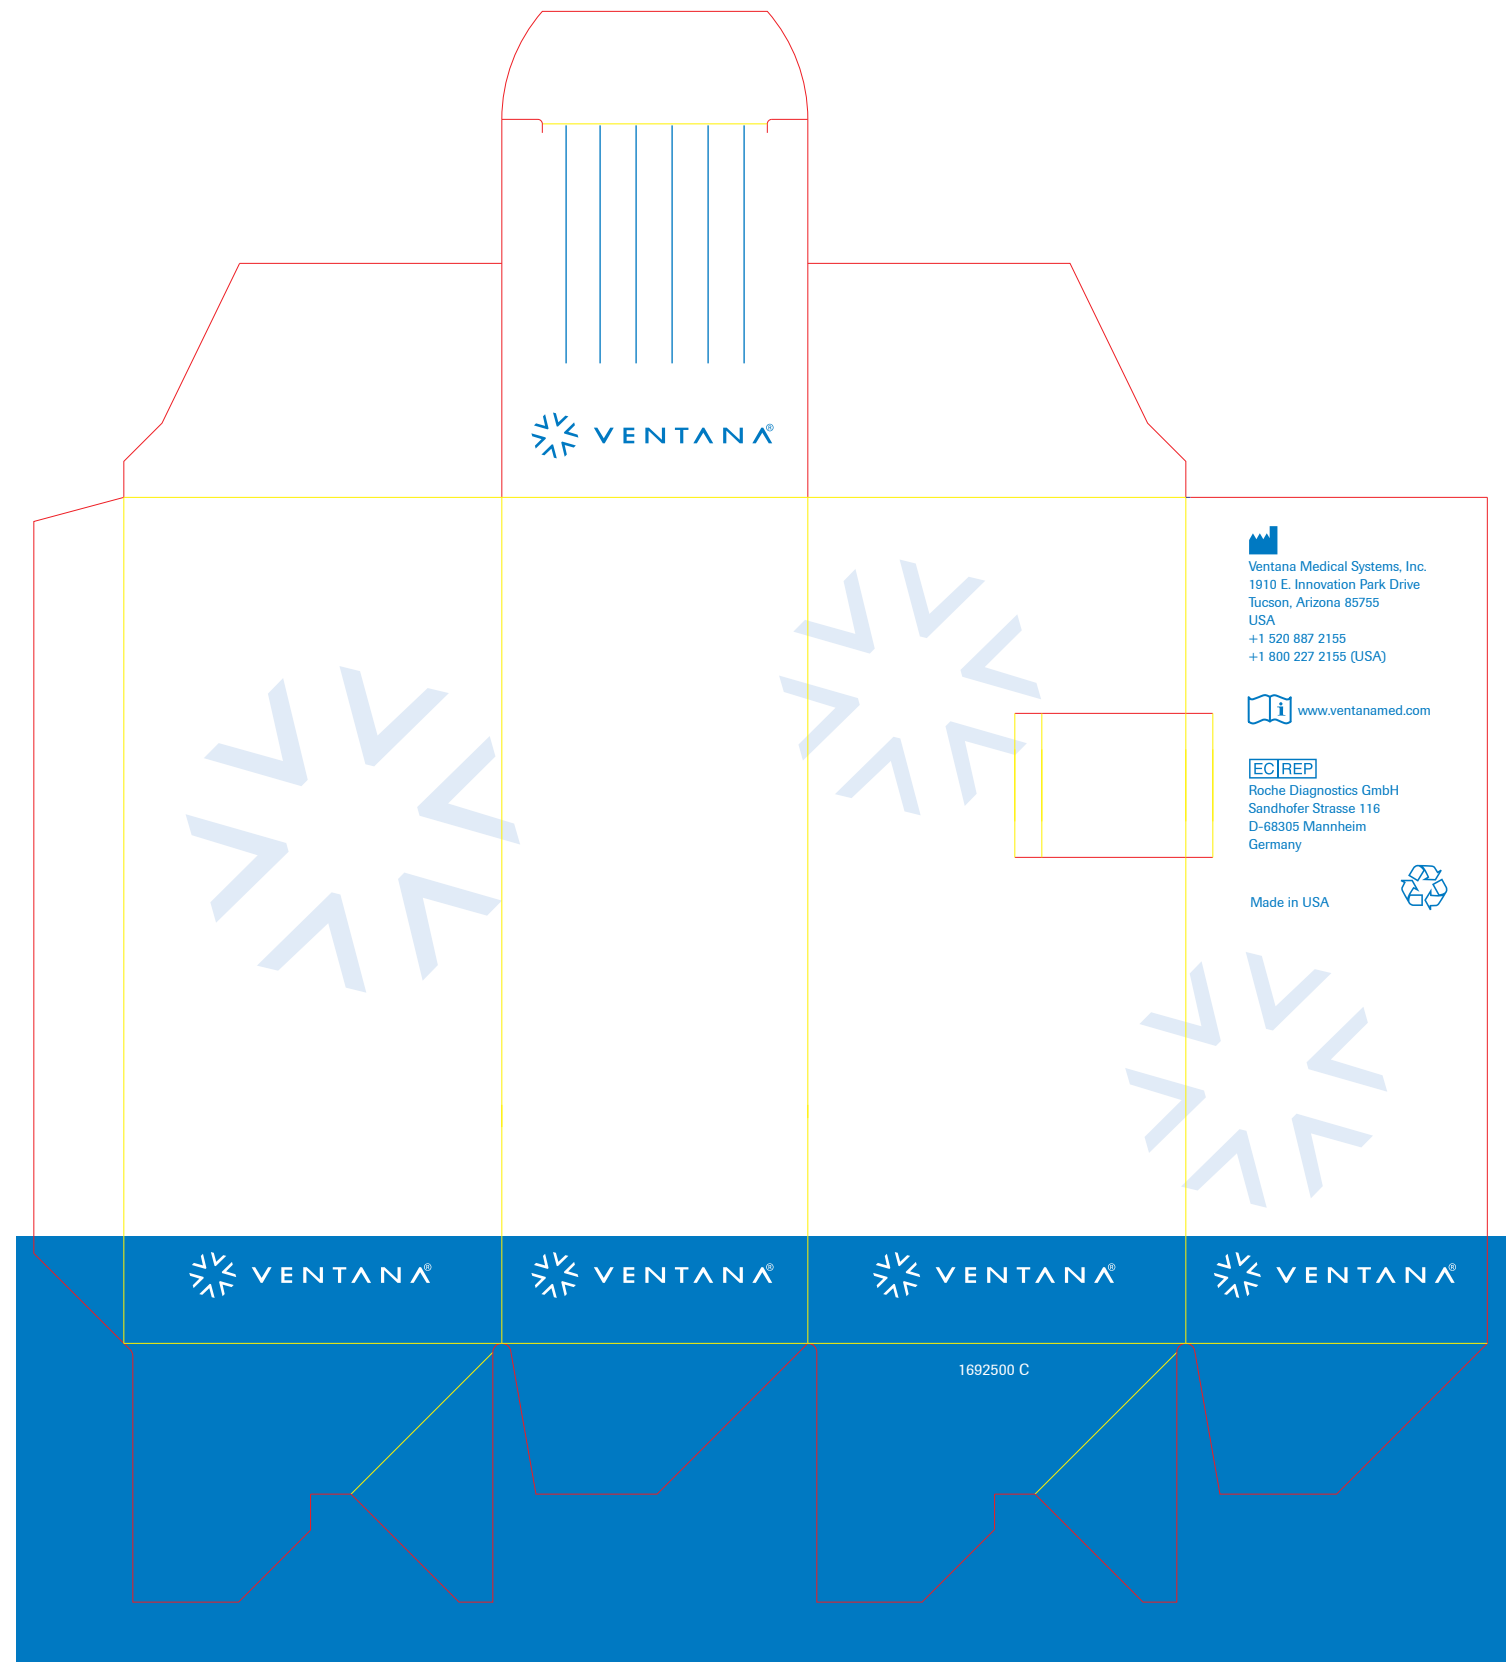

C	UPDATE REV FOR SPEC CHANGE ON VARNISH	SEE AGILE	GV	C007663
B	UPDATE ARTWORK WITH BLUE BORDER	SEE AGILE	PM	C003389
A	RELEASED DRAWING	SEE AGILE	GA	10682
REV	DESCRIPTION	Effective Date	RP	CO
 VENTANA®		Ventana Medical Systems Inc. Tucson, AZ		
TITLE ARTWORK, SINGLE DISPENSER, BOX PN 1692500				
SCALE DO NOT SCALE	SHEET 1 OF 1	SIZE B	DWG NUMBER 000014900	REV C

Nhãn sản phẩm

1. Bluing Reagent (05266769001)

Hóa chất xét nghiệm
Bluing Reagent
(05266769001)

Số lưu hành:

Chủ sở hữu số lưu hành:

Công ty TNHH Roche Việt Nam

Tầng 27, Tòa nhà Pearl Plaza, 561A Điện Biên Phủ, Phường 25,

Quận Bình Thạnh, Tp. Hồ Chí Minh

Nhà sản xuất: Ventana Medical Systems, Inc., 1910 E. Innovation Park Drive, Tucson AZ 85755, Mỹ

Xuất xứ: Mỹ

Hướng dẫn bảo quản: xem 

Số lô: xem LOT - **Hạn sử dụng:** xem  trên bao bì

Hướng dẫn sử dụng xem tại <http://dmec.moh.gov.vn>

Các thông tin khác xem trong hướng dẫn sử dụng

Hỗ trợ kỹ thuật vui lòng liên hệ 1800599991