

**Vật liệu kiểm soát mức thấp, mức trung bình, mức cao xét nghiệm định lượng 18 thông số huyết học
Liquichek Hematology Control (C)**

Số lưu hành:

Quy cách đóng gói: Hộp 3 x 5 mL

Số lô: xem **LOT** trên nhãn gốc

Hạn sử dụng: xem  trên nhãn gốc

Điều kiện bảo quản: Bảo quản ở 2°C đến 8°C

Hướng dẫn sử dụng, cảnh báo thận trọng và các thông tin khác: Tra cứu tại website: myeinserts.qcnet.com

Chủ sở hữu số lưu hành: Công ty TNHH Thương mại Sixmurs HTH Việt Nam

Địa chỉ: Số nhà 9, Ngõ 7, Đường Lê Đức Thọ, Phường Mỹ Đình 2, Quận Nam Từ Liêm, Thành phố Hà Nội, Việt Nam

Cơ sở sản xuất/ Địa chỉ: Bio-Rad Laboratories Inc./ 9500 Jeronimo Road, Irvine, CA 92618, Mỹ

Chủ sở hữu sản phẩm/ Địa chỉ: Bio-Rad Laboratories Inc./ 9500 Jeronimo Road, Irvine, CA 92618, Mỹ

Xuất xứ: Mỹ

Nhà nhập khẩu:




GIÁM ĐỐC
Phạm Thị Thu Hằng

Liquichek™ Hematology Control (C) for R&D Systems

Outside Printing of Vial Label Artwork

BIO-RAD ARTWORK SPECIFICATIONS

UPDATED ON : 7/12/2012
DESKTOP PUBLISHER : Joshua Welles
BIO-RAD LOGO : PMS 347
(Level 1) 2nd COLOR : PMS 300
(Level 2) 2nd COLOR : PMS 347
(Level 3) 2nd COLOR : PMS 485
REMAINING COLOR : Black
LABEL DIMENSIONS : 1-3/4" H x 1-3/8" W
CORNER RADIUS : 0.125" (1/8")
DCR# : 12-0591
COMPONENT SPEC.# : 765225 (RDS spec. #)

BAR CODE SPECIFICATIONS

Code-128 : Optimized General
Resolution : 2400 DPI
Bar Width Reduction : BWR=4
Height : 0.25" H (1/4")
Magnification : 133.33%




EXAMPLE BARCODES (FOR REFERENCE ONLY)

Low Level		0087XXX1
Normal Level		0088XXX2
High Level		0086XXX3




QA APPROVED COPY
7/16/12

GIÁM ĐỐC
 Phạm Thị Thu Hằng

Actual Size

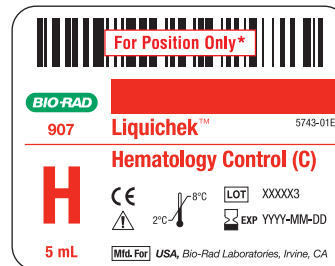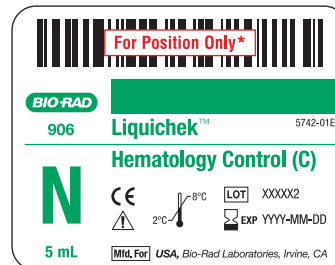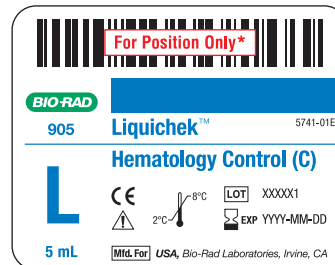

150%

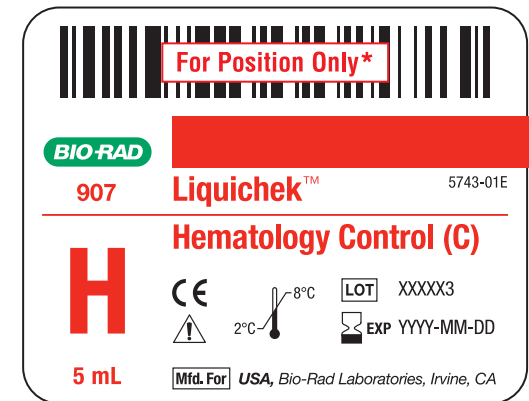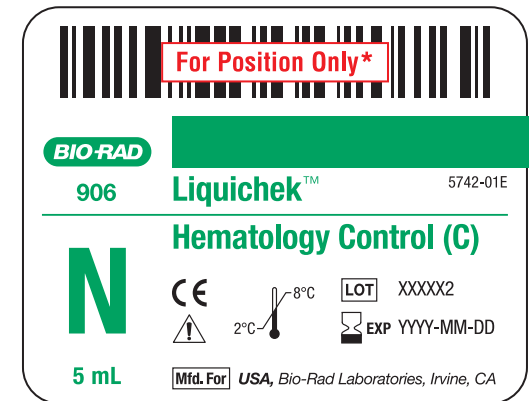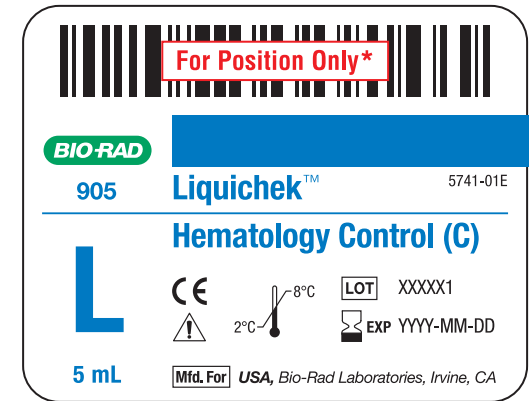

* This bar code specifies Level Number (0087XXX1=LOW, 0088XXX2=NORMAL, 0086XXX3=HIGH) and Lot Number. (XXX is the first 3 digits of the lot number for all levels) The Lot Number and Exp. Date will be provided on the Purchase Requisition. Use this information to generate the bar codes and be sure to maintain the format specified here. The specifications listed above are designated for use on the **Coulter® GEN•S / LH 750 Series** instrument.

Hematology Control (C)**Trilevel
MiniPak**

An assayed hematology control.
 Hämatologiekontrolle mit Zielwertangaben.
 Contrôle d'hématologie titré.
 Controllo dosato per ematologia.
 Control valorado para hematología.
 Um controlo hematológico ensaiado.
 Analyserad hematologisk kontroll.
 En analyseret hæmatologisk kontrol.

**3 x 5 mL
(1 per level)**



(01)XXXXXXXXXXXXXXXXXX
 (17)YYMMDD
 (10)XXX0



LOT XXX0



EXP YYYY-MM-DD



UNITED STATES, Bio-Rad Laboratories
 9500 Jeronimo Road, Irvine, CA 92618



FRANCE, Bio-Rad
 3 boulevard Raymond Poincaré, 92430 Marnes-la-Coquette

ARTWORK SPECIFICATIONS

PART NUMBER : 5399-03ME

1st COLOR : PMS 347

REMAINING COLOR : Black

DIMENSIONS : 4.25"W x 3.667"H