


## MẪU NHÃN

**Bơm tiêm khí máu động mạch có kim**  
**Pro-Vent® Arterial Blood Sampling Kit**  
with Dry Lithium Heparin (Approximately 23 I.U. per ml)

Số lô: xem **LOT**

HSD: xem 

**Hãng, nước sản xuất: Smiths Medical ASD, Inc./USA**

6000 Nathan Lane North, Minneapolis, MN USA

**Hãng, nước chủ sở hữu: Smiths Medical ASD, Inc./USA**

6000 Nathan Lane North, Minneapolis, MN USA

**Nhập khẩu và phân phối bởi: CÔNG TY CỔ PHẦN THIẾT BỊ Y TẾ PT BIOMED**

78/1C Bình Lợi - Phường 13 - Quận Bình Thạnh - TP Hồ Chí Minh, Việt Nam

Cảnh báo, HDSĐ, hướng dẫn bảo quản: xem trong Hướng dẫn sử dụng



GIÁM ĐỐC  
*Nguyễn Thanh Quang*



**SECTION 1 - Unit Artwork:**

Cavity : Size 206.4mm (W) x 57.556mm (H)

Unit designed for Greydon Genesis digital printer.

UNIT LAYOUT (NOT To Scale)

FC10006959-003 1

**STERILE EO**  
Symbol Glossary located in Instructions for Use

**smiths medical portex**

**Arterial Blood Sampling Kit with Dry Lithium Heparin (Approximately 23 I.U. per ml)**

Kit De Prelevement De Sang Arteriel avec De L'heparine Au Lithium Seche (Environ 23 U.I. par ml)  
Arteriellies Blutprobenkit mit Getrocknetem Lithiumheparin (Umgefahr 23 I.E. pro ml)  
Kit Per Il Prelievo Di Sangue Arterioso con Eparina Di Lito Secca (Circa 23 U.I. per ml)  
Juego Para Muestreo De Sangre Arterial con Heparina De Lito Deshidratada (Aproximadamente 23 U.I. por ml)  
Estejo Para Amostragem De Sangue Arterial com Heparina De Lito Desidratada (Aproximadamente 23 U.I. por ml)  
Kit Voor Arteriële Bloedmonsters met Droge Lithiumheparine (Ongeveer 23 I.E. per ml)  
Provtagningssæt For Artaerover med Torr Lithiumheparin (Cirka 23 I.E. per ml)  
Провѣдницьке ТТІ Артерієліє Блѣдгассер мед Вандфрі [Тѳр] Літійумгепарін (Сірка 23 І.Е. пер мл)  
Kit Δεγματοληψίας Αρτηριακού Αιματος με Ξηρό Λιθίου Ηεπαρίνη (Περίπου 23 U.I./ml)

Manufacturer: **Smiths Medical ASD, Inc.**, 6000 Nathan Lane North, Minneapolis, MN 55442 USA [www.smiths-medical.com](http://www.smiths-medical.com)

REF **4629PG**

**Pro-Vent®**  
1ml L/S  
0.6mm x 2.5mm  
(23G x 1 in)

MADE IN USA

CE 2797

COMPOSITE LAYOUT (NOT To Scale)

FC10006959-003

**STERILE EO**  
Symbol Glossary located in Instructions for Use

**smiths medical portex**

**Arterial Blood Sampling Kit with Dry Lithium Heparin (Approximately 23 I.U. per ml)**

Kit De Prelevement De Sang Arteriel avec De L'heparine Au Lithium Seche (Environ 23 U.I. par ml)  
Arteriellies Blutprobenkit mit Getrocknetem Lithiumheparin (Umgefahr 23 I.E. pro ml)  
Kit Per Il Prelievo Di Sangue Arterioso con Eparina Di Lito Secca (Circa 23 U.I. per ml)  
Juego Para Muestreo De Sangre Arterial con Heparina De Lito Deshidratada (Aproximadamente 23 U.I. por ml)  
Estejo Para Amostragem De Sangue Arterial com Heparina De Lito Desidratada (Aproximadamente 23 U.I. por ml)  
Kit Voor Arteriële Bloedmonsters met Droge Lithiumheparine (Ongeveer 23 I.E. per ml)  
Provtagningssæt For Artaerover med Torr Lithiumheparin (Cirka 23 I.E. per ml)  
Провѣдницьке ТТІ Артерієліє Блѣдгассер мед Вандфрі [Тѳр] Літійумгепарін (Сірка 23 І.Е. пер мл)  
Kit Δεγματοληψίας Αρτηριακού Αιματος με Ξηρό Λιθίου Ηεπαρίνη (Περίπου 23 U.I./ml)

Manufacturer: **Smiths Medical ASD, Inc.**, 6000 Nathan Lane North, Minneapolis, MN 55442 USA [www.smiths-medical.com](http://www.smiths-medical.com)

REF **4629PG**

**Pro-Vent®**  
1ml L/S  
0.6mm x 2.5mm  
(23G x 1 in)

MADE IN USA

CE 2797

123456789  
2013-04-11  
2018-04-10  
GTM: 20351688081138

Uncontrolled

f Not Current

**SECTION 2 - Shelf Artwork:**  
 Pre-printed label stock: 276mm (W) x 88mm (H)  
 Label designed to be printed in P360.

The colors represented in this document may not be a true representation of the assigned Pantone color.  
**EXAMPLE LAYOUT (NOT To Scale)**

## Pro-Vent® Arterial Blood Sampling Kit

with Dry Lithium Heparin (Approximately 23 I.U. per ml)

  
**Caution**  
 Keep away from sunlight

  
 Do not reuse

  
 Keep dry

  
 Do not use if package is damaged

  
**STERILE EO** Sterilized using ethylene oxide

  
 Not made with natural rubber latex

  
**2797**

Pro-Vent, Portex and Smiths Medical design marks are trademarks of Smiths Medical.

**USA Manufacturer:**  
 Smiths Medical AG, Inc.  
 6090 Nathan Lane North  
 Minneapolis, MN 55442 USA  
**MADE IN USA**

**EU/UK Representative:**  
 Smiths Medical Europe s.p.a.  
 Copernicus 300, Hradec  
 733 01 Hradec, Czech Republic  
[www.smiths-medical.com](http://www.smiths-medical.com)

Lot: 123456789  
 Exp: 2013-04-11  
 PC10016511-002

smiths medical REF 4629PG  
 portex

**Pro-Vent® Arterial Blood Sampling Kit**  
 23G x 1 in  
 (0.6mm x 25mm)  
 1mL LS

LOT 123456789  
 MW 2013-04-11  
 2018-04-10

smiths medical

  
 (01)10351688081131(11)130411(17)180410(10)123456789

  
 (01)10351688081131(11)130411(17)180410(10)123456789

**SECTION 3 - Transit Artwork:**  
 Pre-printed label stock: 276mm (W) x 88mm (H)  
 Label designed to be printed in P360.

The colors represented in this document may not be a true representation of the assigned Pantone color.  
**EXAMPLE LAYOUT (NOT To Scale)**

## Pro-Vent® Arterial Blood Sampling Kit

with Dry Lithium Heparin (Approximately 23 I.U. per ml)

  
**Caution**  
 Keep away from sunlight

  
 Do not reuse

  
 Keep dry

  
 Do not use if package is damaged

  
**STERILE EO** Sterilized using ethylene oxide

  
 Not made with natural rubber latex

  
**2797**

Pro-Vent, Portex and Smiths Medical design marks are trademarks of Smiths Medical.

**USA Manufacturer:**  
 Smiths Medical AG, Inc.  
 6090 Nathan Lane North  
 Minneapolis, MN 55442 USA  
**MADE IN USA**

**EU/UK Representative:**  
 Smiths Medical Europe s.p.a.  
 Copernicus 300, Hradec  
 733 01 Hradec, Czech Republic  
[www.smiths-medical.com](http://www.smiths-medical.com)

Lot: 123456789  
 Exp: 2013-04-11  
 PC10016519-002

smiths medical REF 4629PG  
 portex

**Pro-Vent® Arterial Blood Sampling Kit**  
 23G x 1 in  
 (0.6mm x 25mm)  
 1mL LS

LOT 123456789  
 MW 2013-04-11  
 2018-04-10

smiths medical


  
 (01)30351688081135(11)130411(17)180410(10)123456789

  
 (01)30351688081135(11)130411(17)180410(10)123456789

**SECTION 4 - Transit and Shelf Carton Label Placement:**

EXAMPLE LAYOUT (NOT To Scale)


**Generic Label Position**

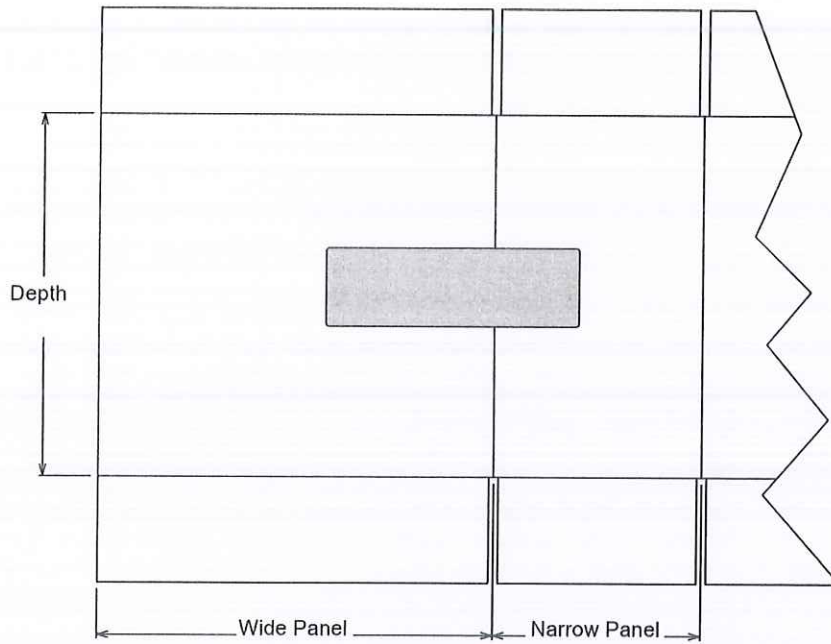

- NOTES:** 1) Label should be positioned centrally within carton/box depth.  
2) Barcode and variable data should be on narrow panel.



**Blank Carton/Box with Label Applied**

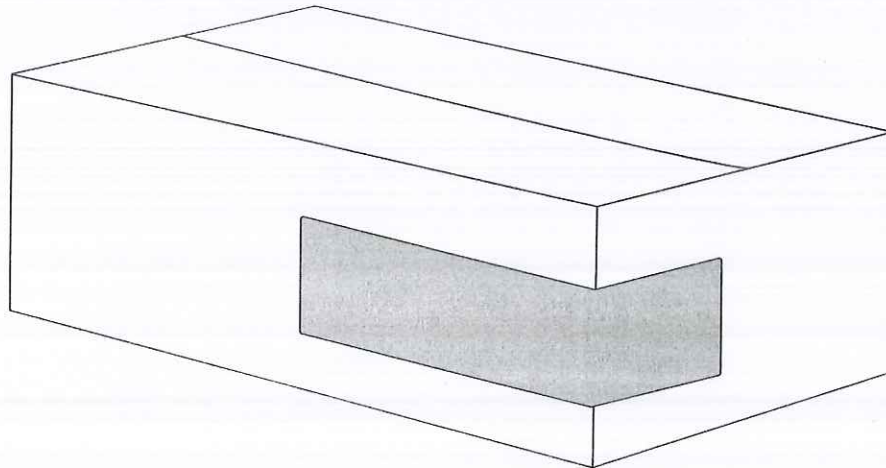

Not Current

Uncontrolled