

VI **REF** 04U45-20

KXXXXV
GXXXX/RXX



Thuốc thử xét nghiệm định lượng Albumin
Albumin BCP2

Số lưu hành: XXXX-XXXX-XXXX

Chủ sở hữu số lưu hành: Văn phòng Đại diện Abbott Laboratories GmbH tại Hà Nội. Địa chỉ: Tầng 7, tầng 8 tháp A, tòa nhà Handi Resco, số 521 Kim Mã, quận Ba Đình, Hà Nội.

Chủ sở hữu trang thiết bị: Abbott Ireland Diagnostics Division. Địa chỉ: Lisnamuck, Longford, Co. Longford, Ireland.

Xuất xứ: Ireland

Số Lô SX và ngày hết hạn: Xem "**LOT**" và "**Exp.**" trên nhãn gốc.


Nhiệt độ bảo quản: 15-30°C

Thông tin cảnh báo, Hướng dẫn sử dụng, Hướng dẫn bảo quản: Xem Hướng dẫn sử dụng kèm theo hộp hoặc tải trên trang www.corelaboratory.abbott/IFU.

AlbBCP2



R1 4 x 15.8 mL



REF 04U4520  4 x 150

 www.corelaboratory.abbott/IFU

 Exp.

LOT

 Abbott Ireland
Diagnostics Division
Lisnamuck, Longford
Co. Longford
Ireland
+353-43-3331000

PRODUCT OF IRELAND




G93184R03

04U45-TF-20_Eng_POTe.indd 1

24-Mar-20 12:24:16

File: 04U45-TF-20_Eng_POTe.indd
Template: ARCH Kit Label.indd
Drawing: AK4727
Size: 125 x 90 mm
UDI Stamp field: 65 X 37 mm
Colors: Text, Logo and Symbols: Black
Abbott A, Lines and Product Name: Pantone 369 C
GHS Colors: Warning Symbol: Border: Pantone 185 c / Inside border Symbol: black
Material: Refer to site specific documents

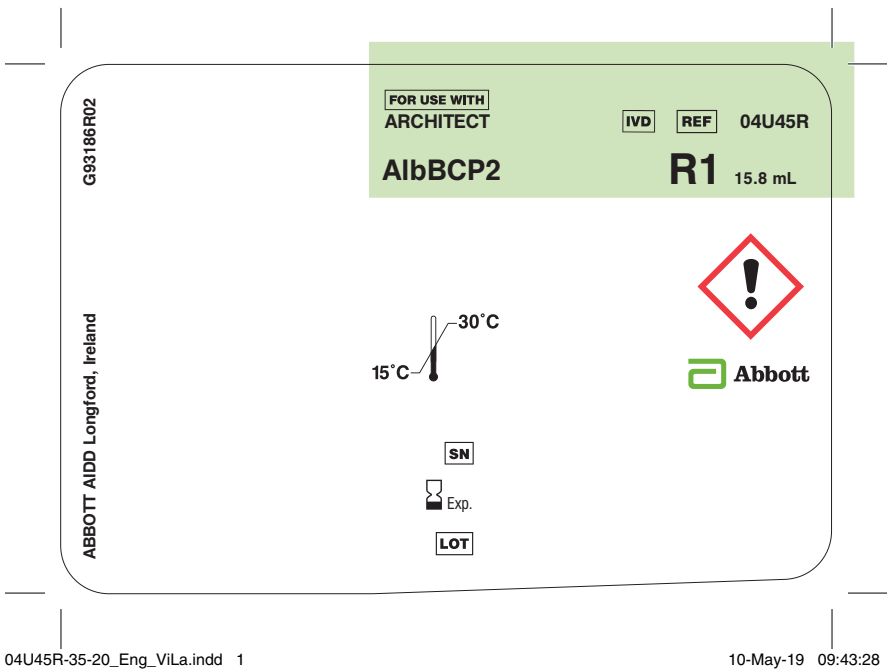

File: 04U45R-35-20_Eng_ViLa.indd
 Template: Wedge Label.indt
 Drawing: AK4743
 Size: 102 x 70 mm
 Stamp field: See Drawing
 Colors: Text and Symbols: Black
 ARCHITECT Symbol: Black
 Color Panel: Pantone 369 C 30%
 Abbott Core Signature: Pantone 369 C and Black

GHS Colors: Warning Symbol: Border: Pantone 185 c / Inside border Symbol: black
Material: Refer to site specific documents