

# MẪU NHÃN


Người đại diện hợp pháp của cơ sở

## *Nhãn phụ:*

**Chất hiệu chuẩn xét nghiệm định lượng HDL**  
**Atellica CH HDLC CAL**

Số lưu hành: xxxx

Số lô: Xem  trên nhãn gốc

Hạn sử dụng: Xem  trên nhãn gốc

Bảo quản: Xem  trên nhãn gốc

Chủ sở hữu TTBYT: Xem  trên nhãn gốc.

Nước chủ sở hữu: Mỹ


Xuất xứ: Nhật Bản

Chủ sở hữu số lưu hành: Công ty TNHH Thiết bị y tế Phương Đông

Địa chỉ: Tầng 04, Tòa nhà D1, ô đất CT2, Khu đô thị mới Kim Văn – Kim Lũ, Phường Đại Kim, Quận Hoàng Mai, Thành phố Hà Nội, Việt Nam.

Cảnh báo, Hướng dẫn sử dụng, Hướng dẫn bảo quản xin xem trên Hướng dẫn sử dụng tại:  
www.xxxx.xxx

**Nhãn gốc:**

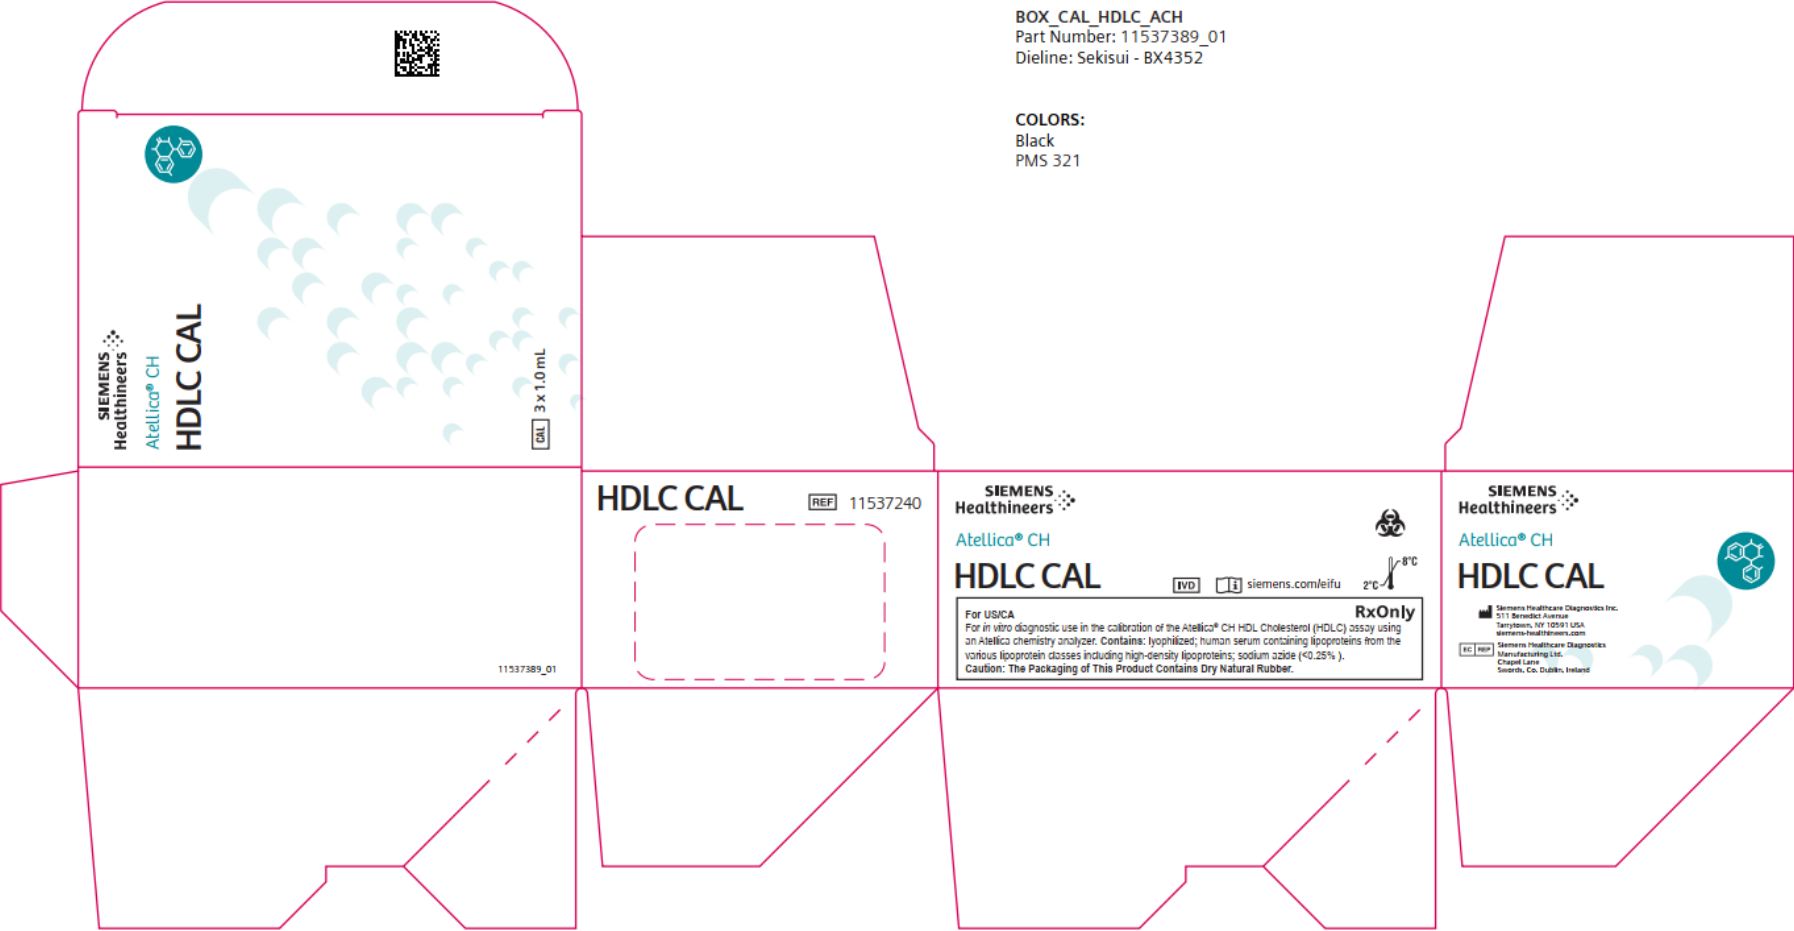

BOX\_CAL\_HDLC\_ACH  
 Part Number: 11537389\_01  
 Dieline: Sekisui - BX4352

COLORS:  
 Black  
 PMS 321

SIEMENS Healthineers  
 Atellica® CH  
**HDLC CAL**  
 3 x 1.0 mL

**HDLC CAL** REF 11537240

SIEMENS Healthineers  
 Atellica® CH

**HDLC CAL**

IVD siemens.com/eifu 2°C 8°C


**RxOnly**  
 For US/CA  
 For in vitro diagnostic use in the calibration of the Atellica® CH HDL Cholesterol (HDLC) assay using an Atellica chemistry analyzer. Contains: lyophilized; human serum containing lipoproteins from the various lipoprotein classes including high-density lipoproteins; sodium azide (<0.25%).  
 Caution: The Packaging of This Product Contains Dry Natural Rubber.

SIEMENS Healthineers  
 Atellica® CH

**HDLC CAL**

Siemens Healthcare Diagnostics Inc.  
 511 Benedick Avenue  
 Tarrytown, NY 10591 USA  
 siemens-healthineers.com  
 Siemens Healthcare Diagnostics  
 Manufacturing Ltd.  
 Chapel Lane  
 Smith, Co. Dublin, Ireland

11537389\_01

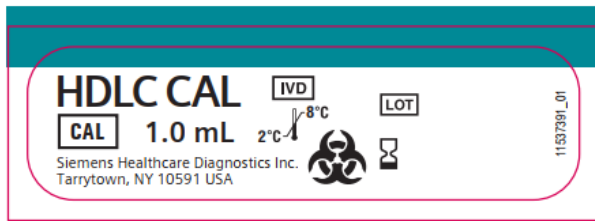

**LABEL\_VIAL\_CAL\_HDLC\_ACH**

Part Number: 11537391\_01

Dimensions: 0.625"H x 2.25"W CR .1875"

**COLORS:**

Black

PMS 321