

SAIO

Serum Proteins Kit 400 Tests

Electrophoresis Procedure

REF SPE42S

Intended use

The Serum Protein Electrophoresis (SPE) kit is intended for the separation of proteins in human serum by electrophoresis on cellulose acetate strips. Human serum proteins are separated into five zones or bands which are composed of many individual proteins. The patterns are examined visually for abnormalities. The kit is used with the automated A Saio instruments.

Summary

Human body fluids contains a varied mixture of proteins and protein complexes. Each of these protein entities apparently fulfills a specific function within the life process; furthermore, it is well known that the levels of various proteins in blood serum bear a close relationship to states of health and disease. In fact, the concentration and compositions of the over one hundred proteins contained in the serum may vary due to physiological conditions. Electrophoresis is a well established and versatile technique, routinely used in clinical laboratories. Serum protein electrophoresis performed at pH 8.8 yields five bands: Albumin and four globulins (alpha 1, alpha 2, beta and gamma). About sixteen of the known proteins contribute to the formation of the five bands in the electrophoretic pattern. Evaluation of single bands by visual inspection provides valuable diagnostic support as it offers a display of the major proteins involved in functional and pathological processes.

Principle

Electrophoresis separates serum proteins based on the premise that the individual protein species have different mobilities when subjected to an electric field. Every molecule possesses an electrical charge due to the presence of positively charged groups and negatively charged groups. The net charge dictates the migration characteristics of the species at a given pH. With the Saio Serum Protein procedure, proteins are separated at an alkaline pH using the principle of Zone Electrophoresis on a suitable support medium: cellulose acetate. When the migration is complete, the proteins are stained and fixed with Ponceau red solution and then washed with a specific destaining solution.

Warning: This kit is for in vitro diagnostic use only.

Specimen Collection and Handling

Serum samples should be collected using the laboratory's procedures and in accordance with Good Laboratory Practice (GLP) Guidelines. Fresh serum samples without hemolysis or lipemia are the optimal choice for testing. Due to interference of fibrinogen, plasma is not recommended. Serum samples may be stored covered at 15°C to 30°C for 4 days or 2°C to 6°C for two weeks, or -20°C for 6 months.

Reagents

Reagents are supplied in concentrated solutions and ready to use. Please reference the operator's manual for the correct addition of reagents to the Instrument reagent rack.

Storage and stability: Store all reagents at room temperature (15°C to 30°C). All reagents are stable until the expiration date indicated on the label.

Strips

Cellulose acetate supported on Mylar®

Buffer (Ready to use solution)

Contains: <10% Tris Base

Staining Solution ready to use

Contains: Ponceau S Red, <5% Acetic acid

Destaining (concentrated solution)

Contains: Citric Acid <50%

Warning: Irritant for eyes and skin

Items Provided

Kit product number: SPE42S For SAIO instrument 400 tests

Ref	Description	Q.ty
AC8C25	Strips - Dry Plates SET	2
BRU52SP	Buffer ready to use 500 mL	1
SRP2AC5	Staining Solution 250 mL	1
DES2AC5	Destaining Solution 250 mL	2
BPS13	Blotting Paper Set for Saio	1

Reagents and Materials Required But Not Provided

- Serological pipettes. Calibrate the pipettes to 20 µL
- Distilled Water.
- Serum Protein Control

Test Procedure

Migration Chamber and Reagents

Insert Blotters in the slots of the migration chamber, insert application paper in the slot of sample holder and put the Dry Strip Paper in the slot for Dry the strip. Complete the preparation of Reagents as indicated on the Operator's Manual. Load diluted Buffer, Ponceau ready to use solution, diluted Destaining solution and Distilled Water in each external tank. Check the level of waste tank, it must be empty.

Strips Positioning

Place the strip on the strip holder as shown in the Operator's Manual. Do not touch the acetate side with fingers.

Samples

Dispense 35 µL of sample into each well of the sample plate. Avoid introducing air bubbles. Bubbles and foam can interfere with results.

Sample Plate

Place the blotter into the correct position as shown in the Operator's Manual. Load the sample plate onto the instrument.

Electrophoresis Conditions

Check on the instrument that the Serum Proteins migration conditions are correct for the specific test. Consult the Operator's Manual for further information on setting.

Start the run

Consult the operator's manual for further information about the starting procedure.


Additional note

The migration chamber papers are good for the duration of the kit
The Dry Strip Paper must be changed after 5 runs of electrophoresis
The Application Paper must be eliminated after 2 cycles.



Test Results

Fig. 1. Normal five fraction serum protein pattern on cellulose acetate. From the start point (cathodic edge) of the cellulose acetate strip to the anode, the bands are: Gamma Globulin, Beta Globulin, Alpha 2 Globulin, Alpha 1 Globulin and Albumin. It should be specified that, with conventional serum proteins dyes, a slight or mild staining of the background between the major fractions may occur due to the presence of lipoproteins, whose protein moieties can bind to the dye. In a normal pattern, Albumin, Alpha 1 and Beta fractions appear to be homogeneous, well shaped bands. Alpha 2 and Gamma fractions are diffuse bands with the Gamma fraction showing a more intensely stained zone in its central part.

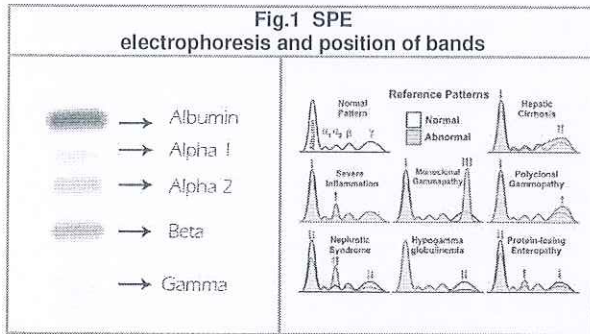

Reference Values

In the following table, the serum reference ranges were established with SPE kit on **Saio** instruments. These values are presented as a guideline. Each laboratory should establish its own reference values.

Fraction	Reference range (%)
Albumin	52.0 - 68.0
Alpha 1	2.0 - 5.0
Alpha 2	6.5 - 13.5
Beta	8.5 - 14.5
Gamma	11.0 - 21.0

Quality control

It is recommended to include controls with the patient sample runs in accordance with the guidelines or requirements of local, state, and/or federal regulations or accrediting organizations. The laboratory should establish acceptance parameters for each lot of control material. If the controls are not within these parameters, patient test results are suspect and the analysis should be repeated.

Bibliography

1. Killingsworth, L.M. et al., Protein Analysis, Diag Med, Jan/Feb., 47-58, 1980
2. Ritzmann, S.E. and Daniels, J.C., Serum Protein Abnormalities: Diagnostic and Clinical Aspects, Little, Alan R. Liss Inc., 1982
3. Aguzzi F, Jayakar SD, Merlini G., Petrini C. Electrophoresis: cellulose acetate vs agarose gel, visual inspection vs densitometry. Clin. Chem. 1981; 27.
4. Merlini G., Aguzzi F. The laboratory investigation of monoclonal components. Haematologica 1988; 73, 79-85.
5. Savoia M., Palmieri D., Guarini R., Oriani G., La Rocca S., Rivisitazione critica del tracciato sieroproteico: contributo sperimentale per la metodologia e le implicazioni fisiopatologiche. Giorn. It. Chim. Clin. Vol. 14, N.1, 1989.
6. Introzzi. Elettroforesi delle sieroproteine su acetato di cellulosa. Trattato Italiano di Medicina, Tecniche di Laboratorio, Vol. IV, 3024-3027, 1970.

The compliance of the kit with the directive 98/79/CE and related performance described in the procedure, are guaranteed only if the products are used according to our instructions of use

SAFETY CLAIMS

1. Before starting the assay, read the instructions completely and carefully. Be sure that everything is understood.
2. Don't mix reagents of different lots. Don't use expired reagents.
3. Follow good laboratory practice and safety guidelines. Wear lab coats, disposable latex gloves and protective glasses.
4. If the reagents contained in the kit have a hazardous label, it may cause eye and skin irritations. MSDS for this product are available upon written request to the manufacturer.
5. Chemicals and prepared or used reagents have to be treated as hazardous waste according to national biohazard and safety guidelines or regulations.

Manufacturer: P.S. ELETTRONICA SRL

Address via Nolana II trav.113, 80045 Pompeii (NA) Italy
Tel. +39 081 863 9760 E-mail info@pselettronica.com

SYMBOLS AND MEANING



PRODUCT CODE




LOT NUMBER



READ THE INSTRUCTIONS



EXPIRATION DATE



STORAGE TEMPERATURE



MANUFACTURER



DO NOT RE-USE



IN VITRO DIAGNOSTIC



CE MARK



GIÁM ĐỐC
Lãng Đỗ Dũng