

Declaration of Conformity




AGFA HEALTHCARE N.V.

Septestraat 27, 2640 Mortsel, Belgium

declares that the product

Name: Drystar 5503
Type/model: 5364/300
Application: General Radiology - Mammography

complies with the requirements of the 93/42/EEC Directive (Medical Device).
For this Class I device the procedures of Annex VII have been applied in order to
mark the device with the CE-label.

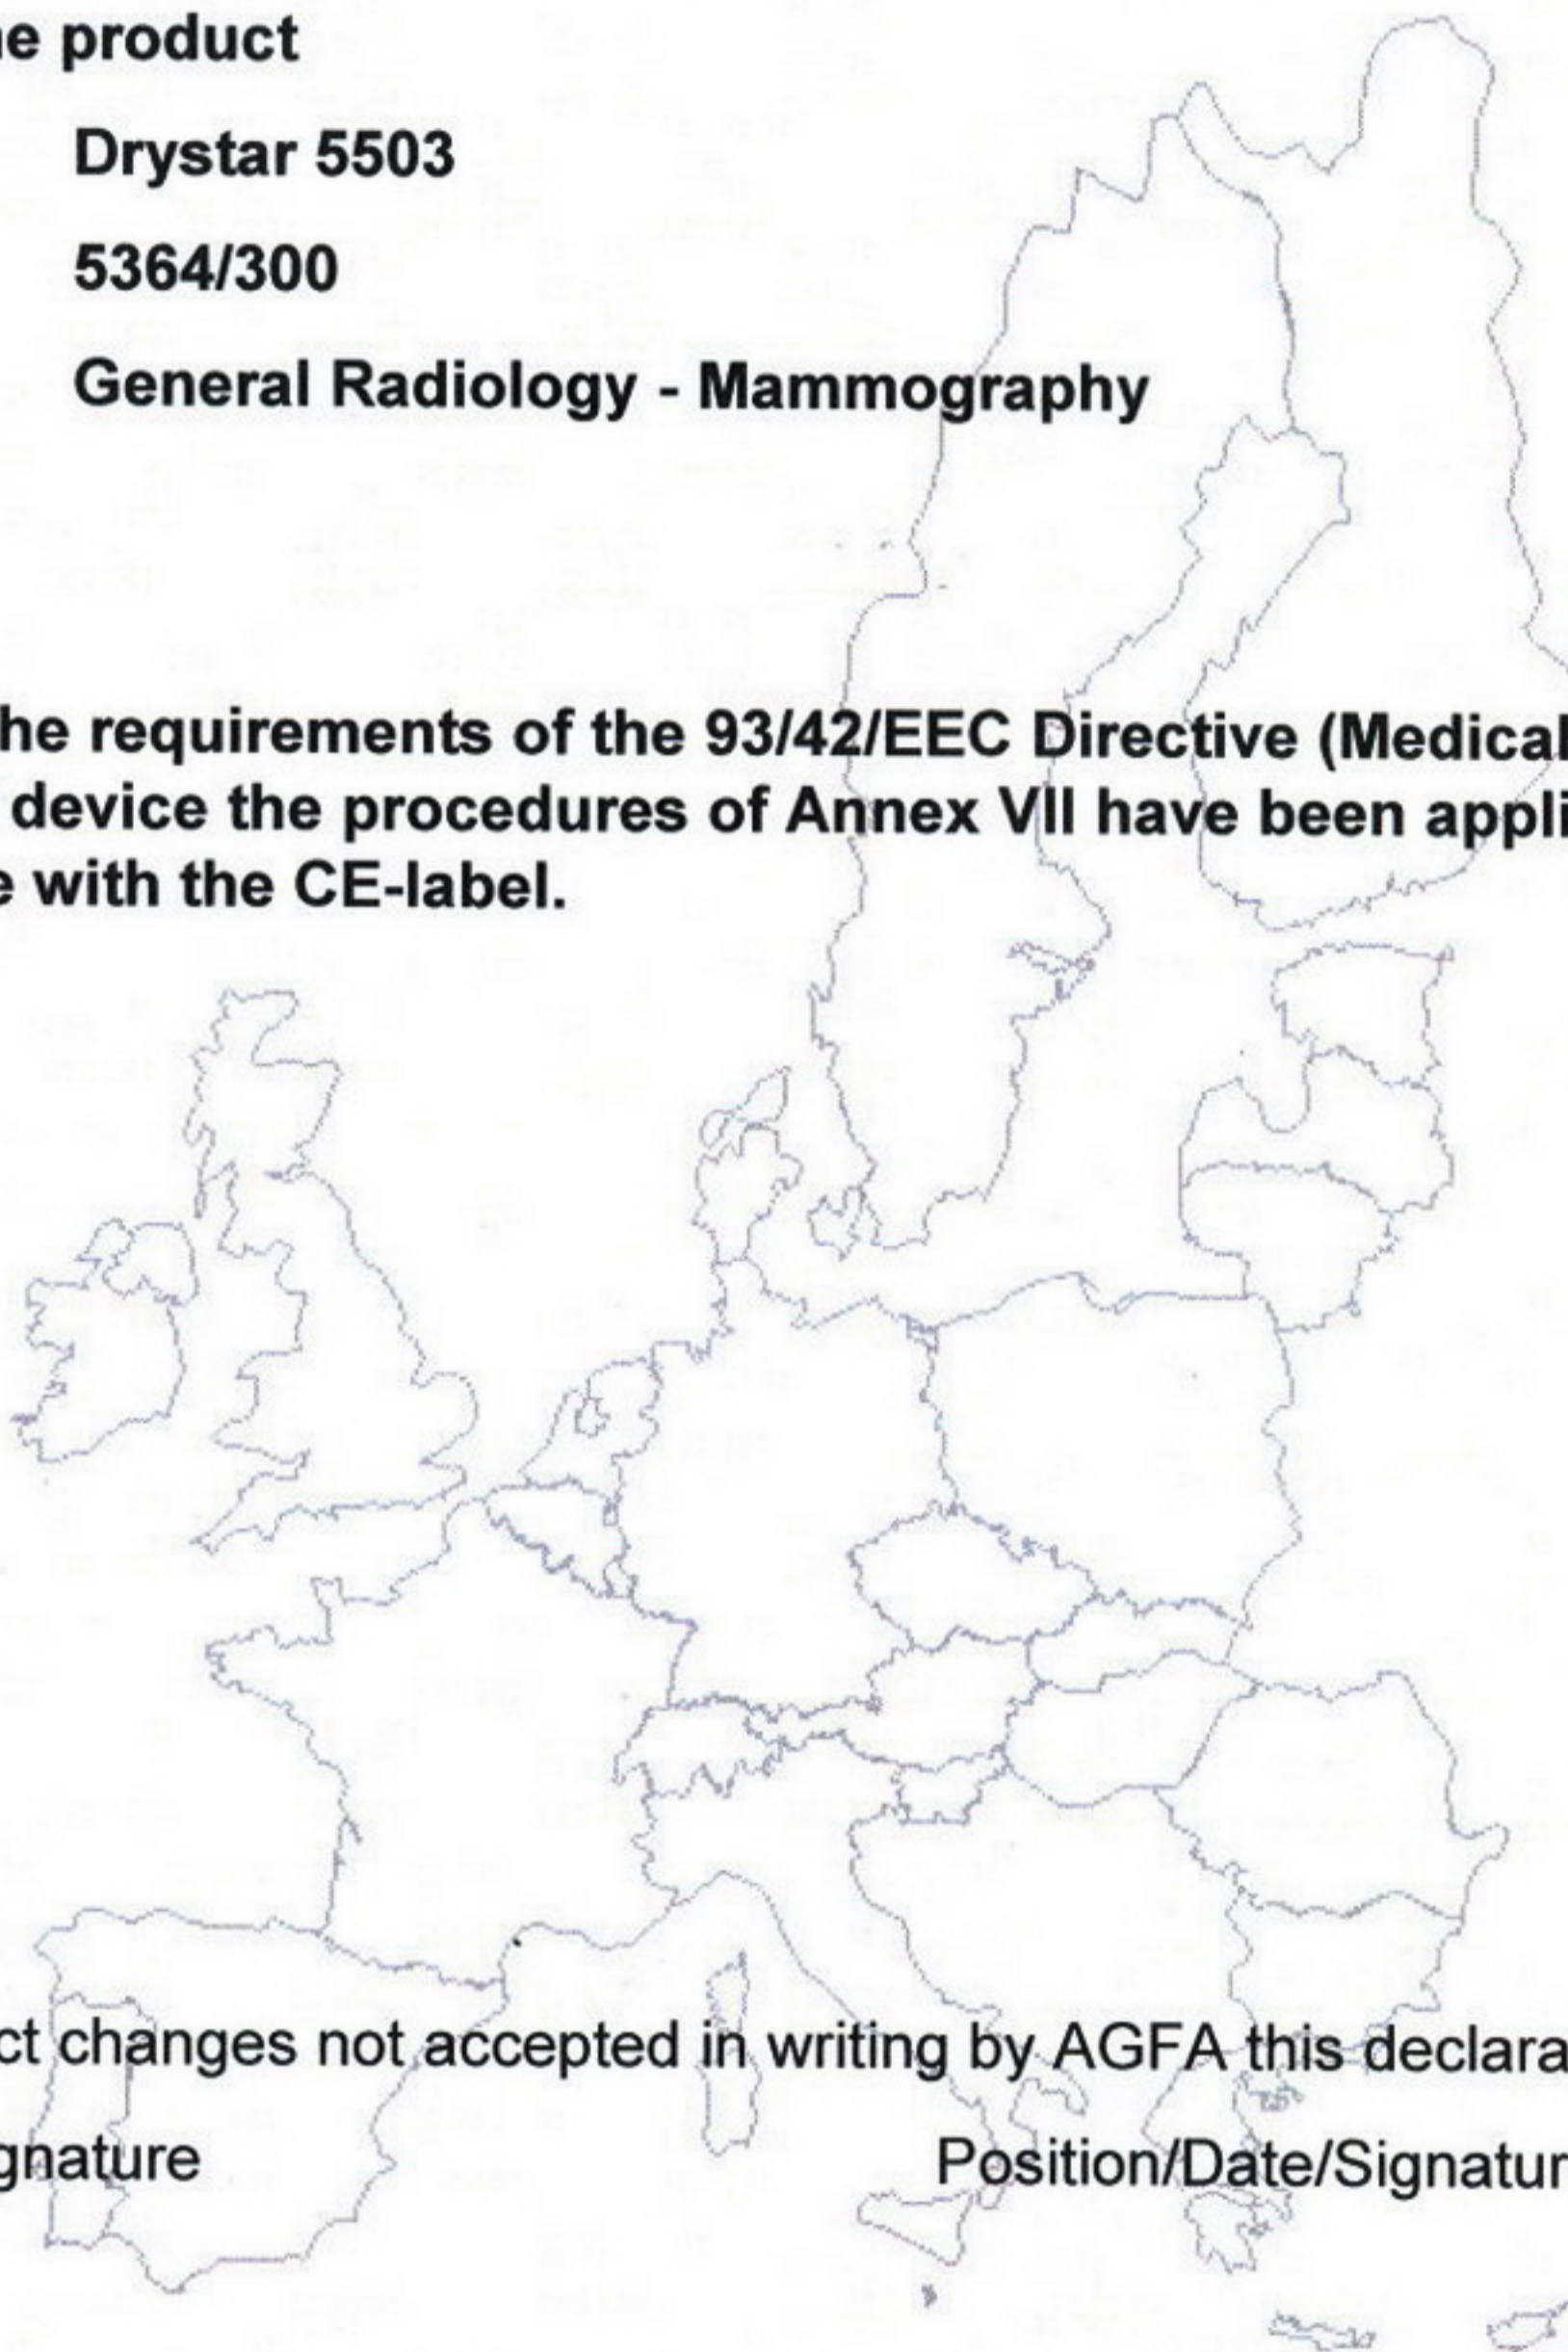


In case of product changes not accepted in writing by AGFA this declaration will expire.

Position/Date/Signature

Position/Date/Signature


30 MAART 2007

Jan Langmans
Manager Global Regulatory
Affairs Agfa HealthCare


30 MAART 2007

Stephen R. Abbott Ph. D.
Vice President, Global Quality Assurance &
Regulatory Affairs Agfa HealthCare